



Analytical Method Development and Validation of Bupropion Metformin and Empagliflozin by RP-HPLC Method

Dr.GOPAL RAO.PAISA, B.INDU,, M.KAVYA, M.SAIKRISHNA

Corresponding Author

Gopal Rao.Paisa

Svs school of pharmacy

HOD pharmaceutical Analysis

Email.id:gopaalrao.paisa@gmail.com



<https://doi.org/10.55041/ijst.v2i7.079>

Cite this Article: RAO.PAISA, G., B.INDU, , M.KAVYA, & M.SAIKRISHNA, (2026). Analytical Method Development and Validation of Bupropion Metformin and Empagliflozin by RP-HPLC Method. International Journal of Science, Strategic Management and Technology, 02(7), 1-9.
<https://doi.org/10.55041/ijst.v2i7.079>

License:  This article is published under the Creative Commons Attribution 4.0 International License (CC BY 4.0), permitting use, distribution, and reproduction in any medium, provided the original author(s) and source are properly credited.

ABSTRACT

A novel very rapid, sensitive, reverse phase High Performance Liquid Chromatography (RP-HPLC) technique was developed for the quantitative estimation of Bupropion in bulk and tablet dosage form. It was resolved by using a mobile phase Potassium di-hydrogen phosphate: methanol in the ratio (60:40 v/v) at a flow rate of 0.8mL/min. using UV - Visible detector at the wavelength of 228 nm for quantification. Efficient separation was achieved for Bupropion on used Waters Acquity HSS T-3 C₁₈ (100 × 2.1 mm, 5µm). The retention time of Bupropion was 2.433min. The calibration graphs were linear and the method showed excellent recovery for tablet dosage form. The developed method was validated according to the International Conference on Harmonization (ICH) guidelines with respect to linearity, accuracy, precision, specificity and robustness.

KEY WORDS: Bupropion, HPLC, new method development, validation

1. INTRODUCTION

Bupropion selectively inhibits the neuronal reuptake of dopamine, nor epinephrine, and serotonin; actions on dopaminergic systems are more significant than imipramine or amitriptyline whereas the blockade of nor epinephrine and serotonin reuptake at the neuronal membrane is weaker for Bupropion than for tricyclic antidepressants¹. The increase in nor epinephrine may attenuate nicotine withdrawal symptoms and the increase in dopamine at neuronal sites may reduce nicotine cravings and the urge to smoke. Bupropion exhibits moderate ant cholinergic effects.²

Structure of drug

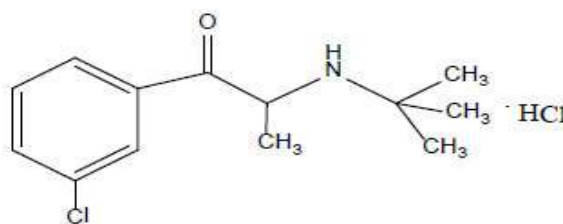


Figure 1: Structure of Bupropion

2. EXPERIMENTAL DETAILS

2.1 Materials and Reagents: Bupropion Working Standard was procured from Teena laboratories, Hyderabad, India. Commercially available Bupropion purchased from local pharmacy. Methanol HPLC Grade and Ortho phosphoric acid AR grade were obtained from Merck chemicals, Mumbai. Water was prepared by using Millipore Milli Q Plus water purification system.

2.2 Chromatographic conditions: Chromatography separation was performed on LC Solution HPLC with UV detector. The output signal was monitored and processed using Chrome- work station HPLC V4.0 software. The chromatographic column used Acquity HSST C₁₈, 50mm × 2.1 mm, 1.7μm column. The mobile phase Potassium di-hydrogen phosphate: methanol in the ratio (60:40 v/v) in the ratio (40:60 v/v) at a flow rate of 0.8mL/min. The detection was monitored at the Wavelength of at 228 nm nm. The injection volume was 20.0 μL and the chromatographic runtime of 5 min was used.

2.3 Preparation of solutions

2.3.1 Preparation of Phosphate buffer: : Weigh 7.0 grams of Potassium di hydrogen phosphate into a 1000ml beaker, dissolve and diluted to 1000ml with milli pore water. Adjusted the pH to 4.0 with ortho phosphoric acid.

2.3.2 Preparation of mobile phase: Mix a mixture of above buffer 600mL (60%) and 400 mL of methanol (40%) and degas in ultrasonic water bath for 5 minutes. Filter through 0.45 μ filter under vacuum filtration.

2.4 Preparation of the Bupropion Standard and sample Solution:

2.4.1 Standard Solution Preparation. Accurately transferred 10mg of Bupropion working standard into a 10 mL volumetric flask and about 7 mL of Diluent added then sonicated to dissolve it completely and the volume was made up to the mark with the same solvent (Stock solution). Further pipette 5 ml of the above stock solution into a 50mL volumetric flask and diluted up to the mark with diluents. Mix well and filter through 0.45 μ m filter. Further pipette 3 ml of the above stock solution into a 10ml volumetric flask and dilute up to the mark with diluents. Mix well and filter through 0.45 μ m filter.

2.4.2 Sample Solution Preparation: Accurately transferred the sample equivalent to 10 mg of Bupropion into a 10 mL volumetric flask. About 7 mL of diluent added and sonicated to dissolve it completely and the volume is made up to the mark with diluents. Mixed well and filtered through 0.45 μ m filter. Further pipette 5 ml of the above stock solution into a 50mL volumetric flask and diluted up to the mark with diluents. Mix well and filter through 0.45 μ m filter. Further pipette 3 ml of the above stock solution into a 10ml volumetric flask and dilute up to the mark with diluents. Mix well and filter through 0.45 μ m filter.

2.5 Method validation

2.5.1 Precision: The precision of the method was evaluated by carrying out six independent assays of test sample against a qualified reference standard and the %RSD of assay was calculated (% RSD should not be more than 2%).

2.5.2 Intermediate Precision/Ruggedness:

2.5.2.1 Intra-day precision: The precision of the assay method was evaluated by carrying out six independent assays Bupropion (50,100, 150% i.e. 5.0, 10.0, 15.0 μ g/Mr.) test samples against qualified reference standard. The percentage of RSD of six assay values was calculated.

2.5.2.2 Intermediate precision (inter-day): Different analyst from the same laboratory and by using different column of same brand evaluated the intermediate precision of the method. This was performed by assaying the six samples of Bupropion against qualified reference standard. The percentage of RSD of six assay values was calculated. The %RSD for the area of six replicate injections was found to be within the specified limits (% RSD should not be more than 2%).

2.5.3 Accuracy: Recovery of the assay method for Bupropion was established by three determinations of test sample using tablets at 50%, 100% and 150% of analyse concentration. Each solution was injected thrice (n=3) into HPLC system and the average peak area was calculated from which Percentage recoveries were calculated. (% Recovery should be between 98.0 to 102.0%).

2.5.4 Linearity: Test solutions were prepared from stock solution at 5 concentration levels (10, 20, 30, 40 and 50 $\mu\text{m}/\text{mol}$). The peak area vs concentration data treated by least square linear regression analysis. (Correlation coefficient should be not less than 0.999.)

2.5.5 Limit of Detection (LOD) Limit of Quantification (LOQ): LOD and LOQ for the were determined at signal to noise ratios of 3:1 and 10:1, respectively by injecting series of dilute solutions with known concentrations

2.5.6 Robustness: To prove the reliability of the analytical method during normal usage, some small but deliberate changes were made in the analytical method (e.g., flow rate, column temperature, and mobile phase composition). Changes in the chromatographic parameters (i.e., theoretical plates and the tailing factor) were evaluated for the studies.

3. RESULTS

3.1 Method development: Different chromatographic conditions were experimented to achieve better efficiency of the chromatographic system. Parameters such as mobile phase composition, wavelength of detection, column, column temperature, pH of mobile phase, and diluents were optimized. Several proportions of buffer, and solvents (water, Phosphate buffer and acetonitrile) were evaluated in order to obtain suitable composition of the mobile phase. Choice of retention time, tailing, theoretical plates, and run time were the major tasks while developing the method. Potassium di-hydrogen phosphate: methanol in the ratio (60:40 v/v) ratio of the mobile phase, a perfect peak was eluted. Thus the mobile phase ratio was fixed at 60:40 (Potassium di-hydrogen phosphate: methanol) in an isocratic mobile phase flow rate. The typical chromatogram obtained for from final HPLC conditions are depicted in Figure2.

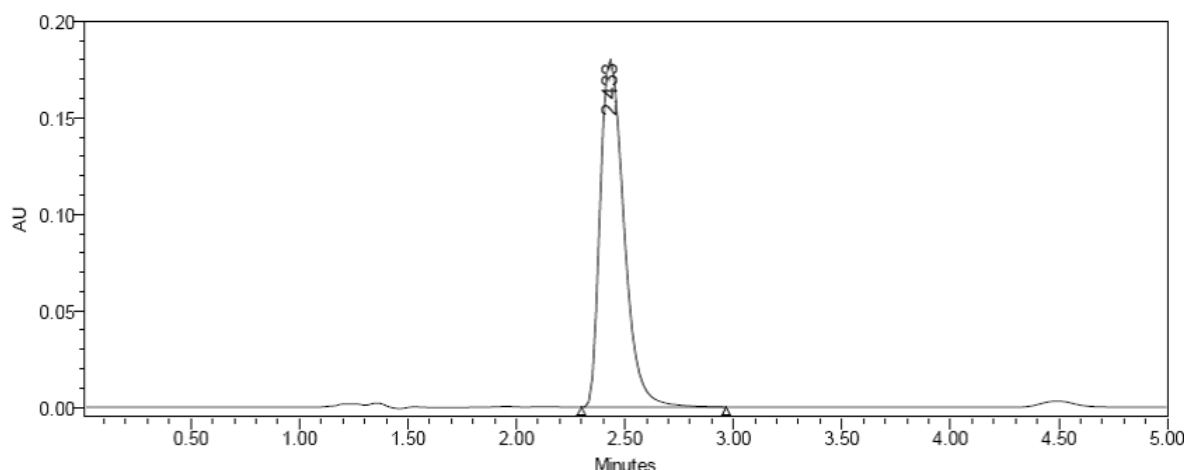


Figure 2: typical chromatogram of by proposed method

3.2 Method validation: Based on International Conference on Harmonization (ICH) guidelines, the method is validated with regard to system suitability, linearity, accuracy, precision, LOD, LOQ, robustness and sensitivity as follows.

3.2.1 System suitability: The system suitability results for the proposed HPLC method are Tailing factor Obtained from the standard injection is 1.4. Theoretical Plates Obtained from the standard injection is 4184.7. The results proved that the optimized HPLC method fulfils these requirements within the USP accepted limits indicated in the 'Experimental' section.

3.2.2 Precision: The % R.S.D. of Bupropion assay during the method precision was found to be 0.45%, indicating good precision of the method. The results are summarized in table 1.

Table 1- Results of precision

Injection	Area
Injection-1	696977
Injection-2	696531
Injection-3	696214
Injection-4	695535
Injection-5	696708
Average	696393
Standard deviation	8624.7
%RSD	1.1%

3.2.4 Limits of detection (LOD) and quantification (LOQ): LOD and LOQ for Bupropion were 0.024 and 0.07 µg/ml, respectively. Since the LOQ and LOD values of Bupropion are achieved at a very low level, this method can be suitable for cleaning validation in the pharmaceutical industry.

3.2.5 Accuracy: Percentage recovery of Bupropion samples ranged from 99.69 % to 101.2% and the mean recovery is 100.5%, showing the good accuracy of the method. The result is shown in Table 3.

Table 3 - Results of Accuracy

%Concentration (at specification Level)	Mean Peak Area (n=3)	Amount Added (mg)	Amount Found (mg)	Average % Recovery	Mean Recovery
50%	688287	5.68	5.78	100.9%	100.7%
100%	1378200	10.0	9.97	99.7%	
150%	2065480	14.05	13.93	98.2%	

3.2.6 Linearity: The linearity of the calibration plot for the method was obtained over the calibration ranges tested, i.e. 10 - 50 µg/ml for three times, and the correlation coefficient obtained was 0.999, thus indicating excellent correlation between peak areas and concentrations of the analyte.

3.2.7 Robustness: In all the deliberately varied chromatographic conditions in the concentration range for the evaluation of robustness is 10 - 50 µg/ml, (n=3). It can be concluded that the variation in flow rate and the variation in 10% Organic composition do not affect the method significantly. Hence it indicates that the method is robust even by change in the flow rate $\pm 10\%$ and change in the Mobile phase $\pm 10\%$. The results are summarized in table 4.

Table- 4- Results of Robustness

<i>Chromatographic changes</i>	<i>USP Plate Count</i>	<i>USP Tailing</i>
Flow rate(ml/min)		
0.6	4187.6	1.5
0.8*	4184.7	1.3
1.0	4084.7	1.4
Change in organic composition in the mobile phase		
10% less	4194.5	1.5
60:40(Buffer: methanol)*	3156.0	1.3
10% more	3097.0	1.4
UV wavelength(nm)		
226	4205.0	1.5
228*	3648.3	1.3
230	3354.2	1.4

3.2.7 Application of the developed method to commercial Bupropion tablets: When the developed method was used to analyze a commercial brand of Bupropion tablet formulation, the mean recovery of triplicates was 99.69 % with % R.S.D. of 0.52. The % recovery value indicates non-interference from the excipients present in the dosage form

DISCUSSION:

Method development and optimization: The main aim of the developed method was to achieve separation and quantification of Bupropion using an isocratic mobile phase with HPLC system. Developing a HPLC method was to reduce the run time of the method and solvent consumption for routine analysis such as assay, dissolution and content uniformity during quality assurance. Detection of Bupropion was adequate at 228 nm. The initial trial was conducted using HPLC and chromatographic separation was obtained on Waters Acquity HSS T-3 C₁₈ (100 × 2.1 mm, 5µm). The mobile phase was Potassium di-hydrogen phosphate: methanol in the ratio (60:40 v/v) at a flow rate of 0.8ml/min. While developing the HPLC method, basic chromatographic conditions such as the used Waters Acquity HSS T-3 C₁₈ (100 × 2.1 mm, 5µm) column, solvents and UV detection employed in the HPLC method were taken into account. In selecting the HPLC column, its stability at the lower pH was taken into consideration to preserve the long life of the column. Most commercial C₁₈ columns are not stable at lower pH on the longer run, thus shortening their life span. Column was found to be more suitable and stable at this pH. The peak was sharp and acceptable. The flow rate also is scaled down from 2.0 to 1.0 ml/min. When these operating conditions were applied to the developed method, a satisfactory peak was achieved for Bupropion which eluted at around 2.433 min giving a total run time of 5 min.

4. CONCLUSION: The new, isocratic RP-HPLC method proved to be simple, linear, precise, accurate, robust, rugged and rapid. The developed method was capable of giving faster elution, maintaining good separation more than that achieved with conventional HPLC. The short retention time of 2.433 min allows the analysis of a large number of samples in a short period of time and is therefore more cost-effective for routine analysis in the pharmaceutical industries. It is suitable for rapid and accurate quality control of Bupropion in tablet formulations.

References:

1. Lovekesh Mehta, and Jitender Singh., RP-HPLC Method Development and Validation for the Determination of Bupropion Hydrochloride in a Solid Dosage Form. RRJPA: Volume 2 Issue 3 July – September, 2013, 1-5
2. M. A. Sameer Abdulaziz, K. Basavaiah; K. B. Vinay. . (2008). Titrimetric and spectrophotometric assay of bupropion hydrochloride in pharmaceuticals using mercury(II) nitrate. Anal. Chem. 80 (), 1756.
3. Sevgi Tatar Ulu1 and Muzaffer Tuncel. (2012). Determination of Bupropion Using Liquid Chromatography with Fluorescence Detection in Pharmaceutical Preparations, Human Plasma and Human Urine. Journal of Chromatographic Science; 50:433–439.